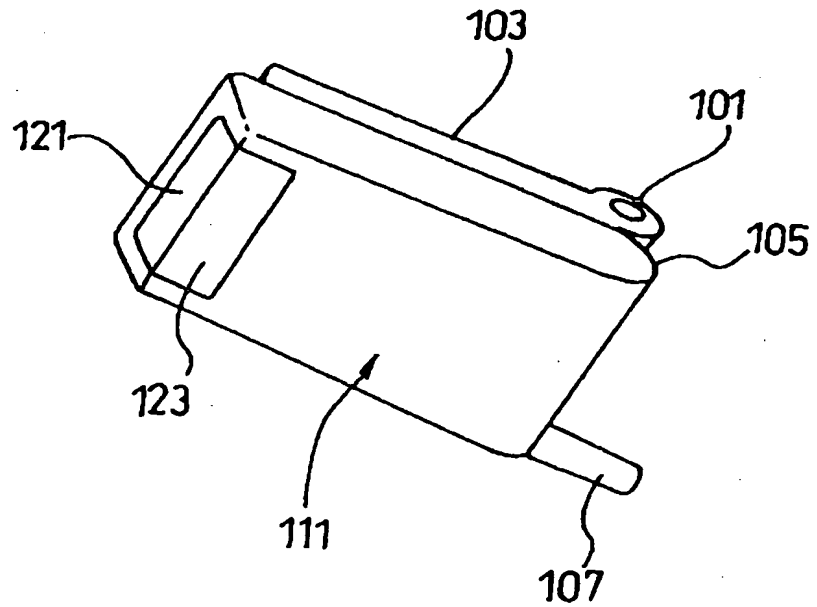
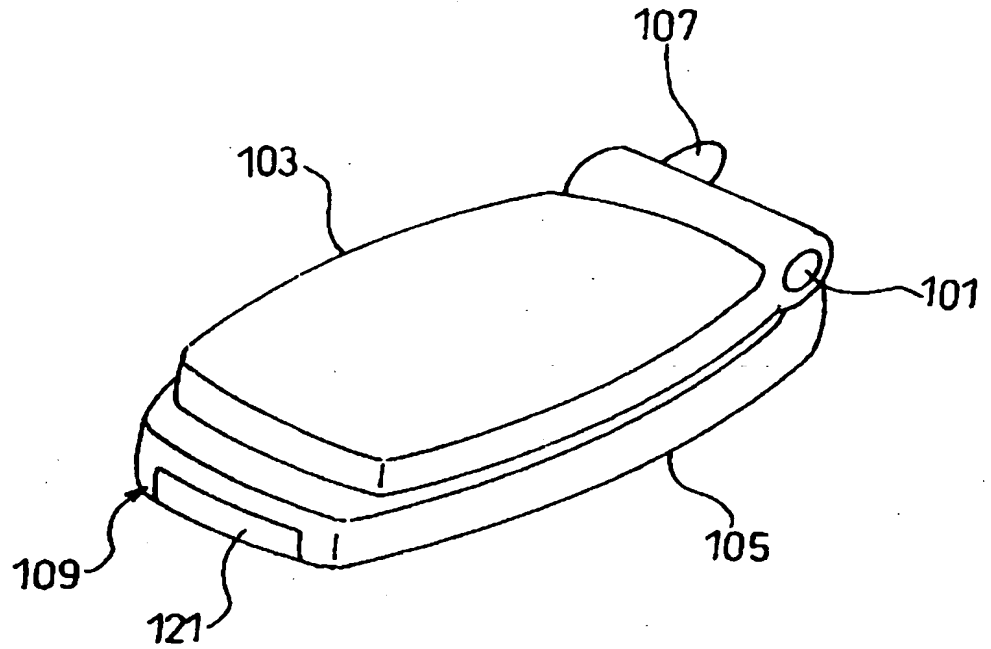


1/11

FIG. 1



**FIG. 2**


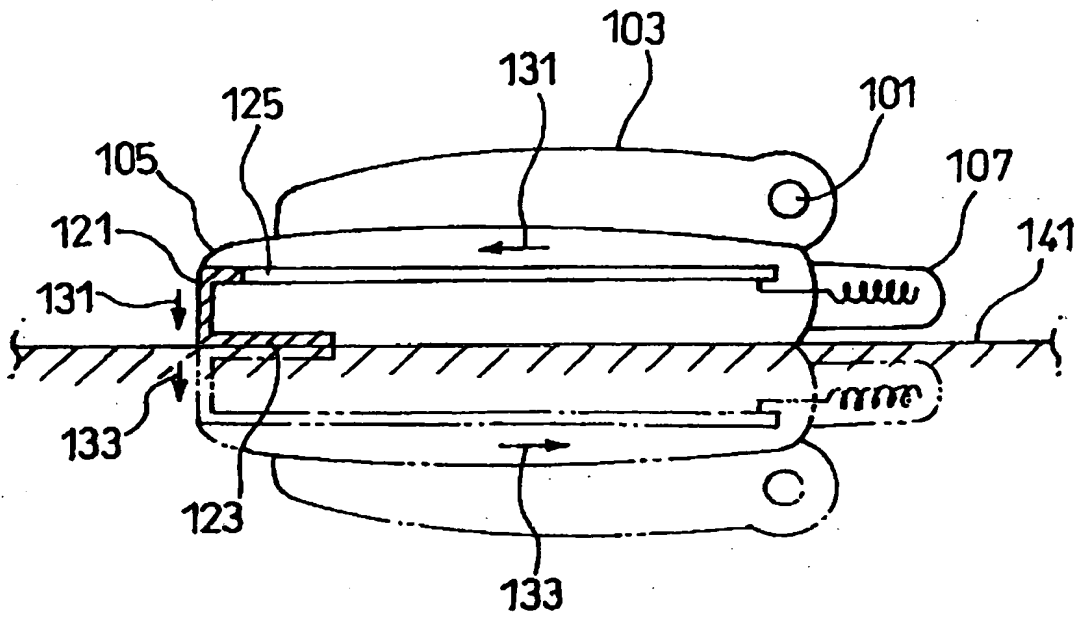


FIG. 3

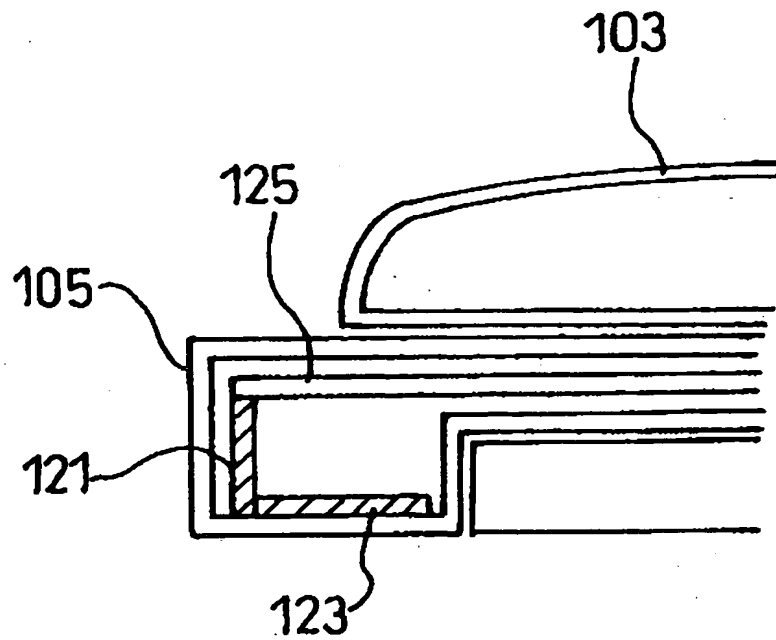

4/11

FIG. 4


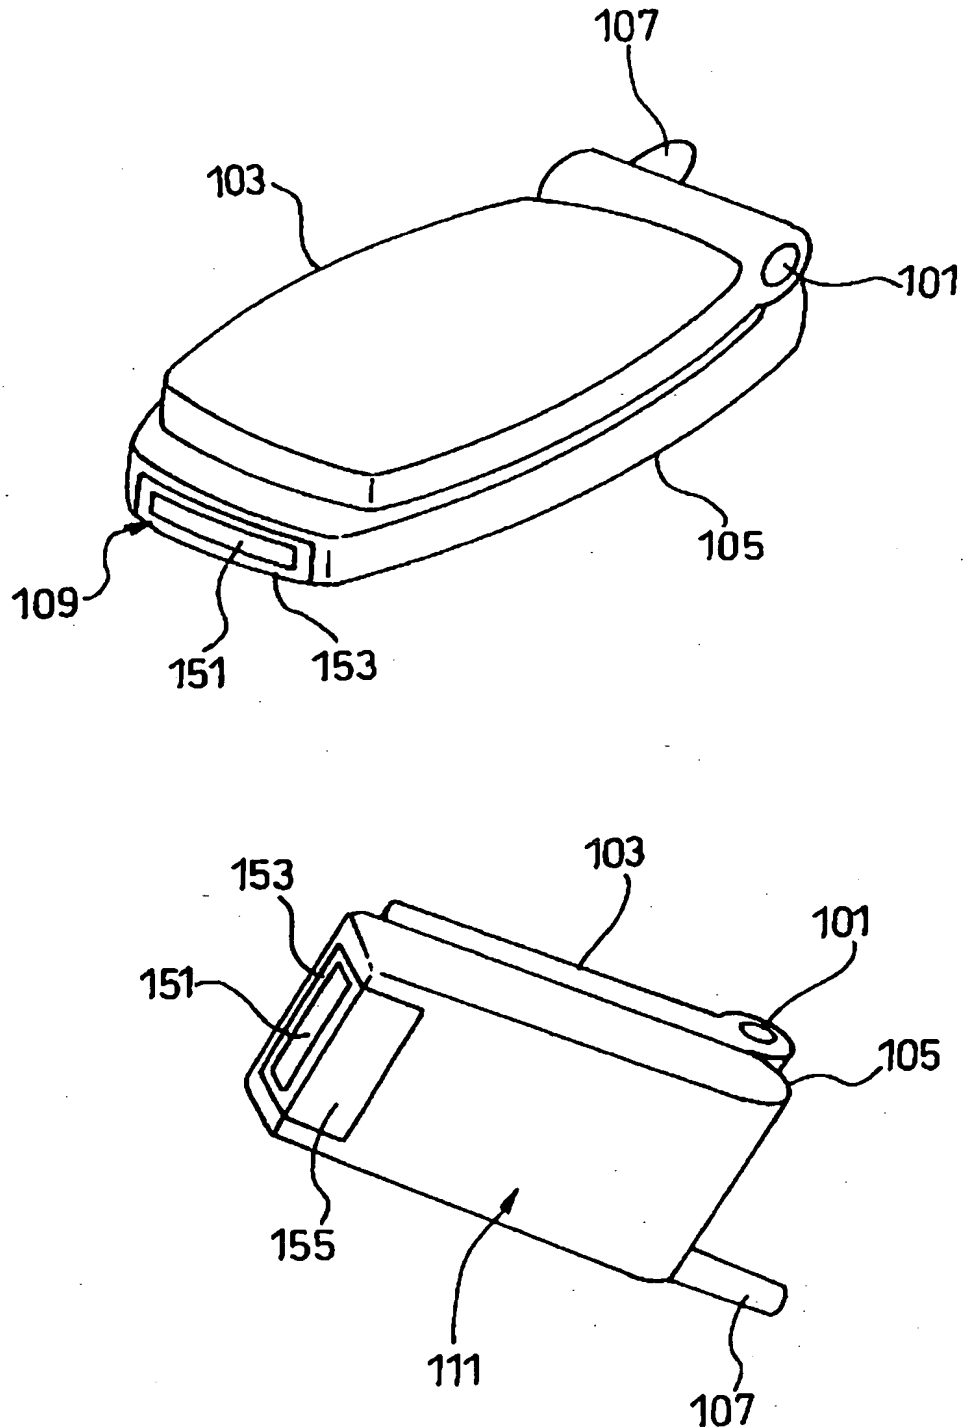


FIG. 5

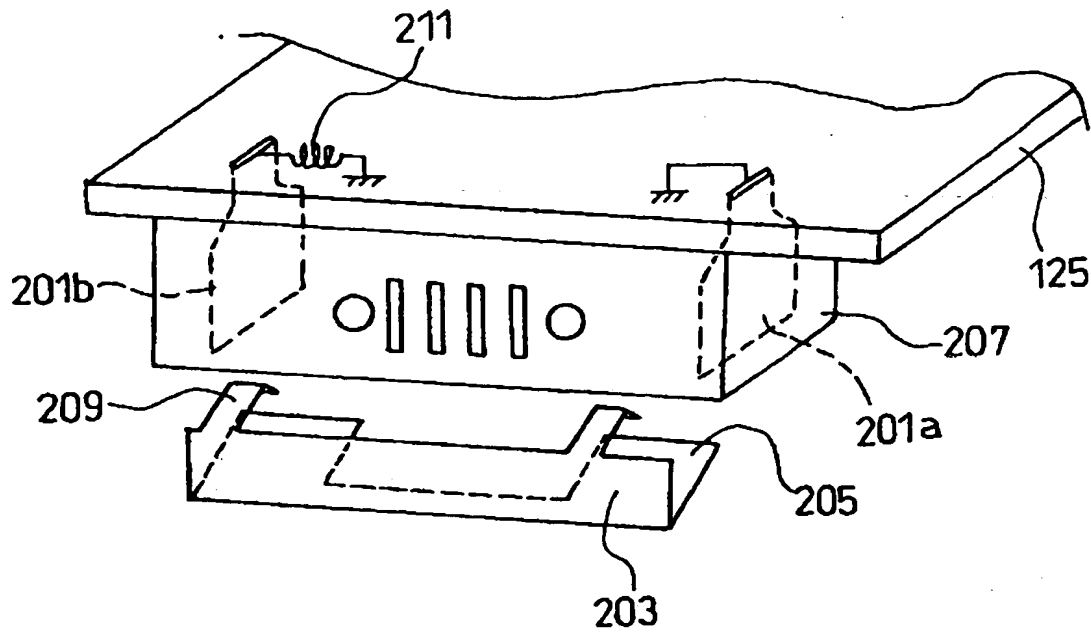

6/11

FIG. 6 (a)

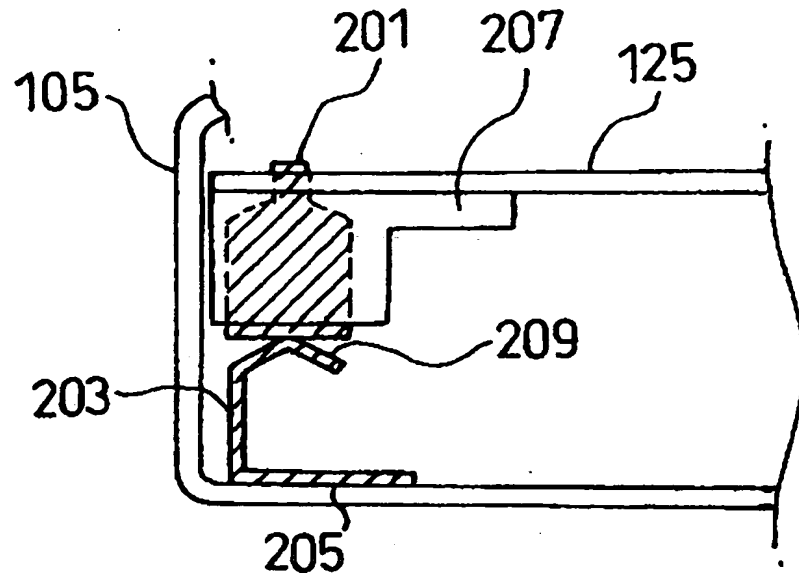


FIG. 6 (b)



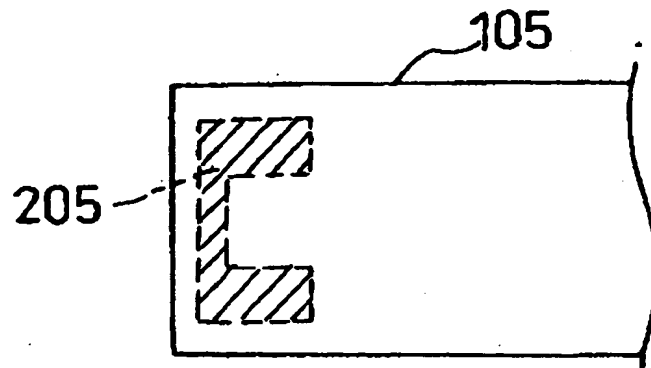


FIG. 7

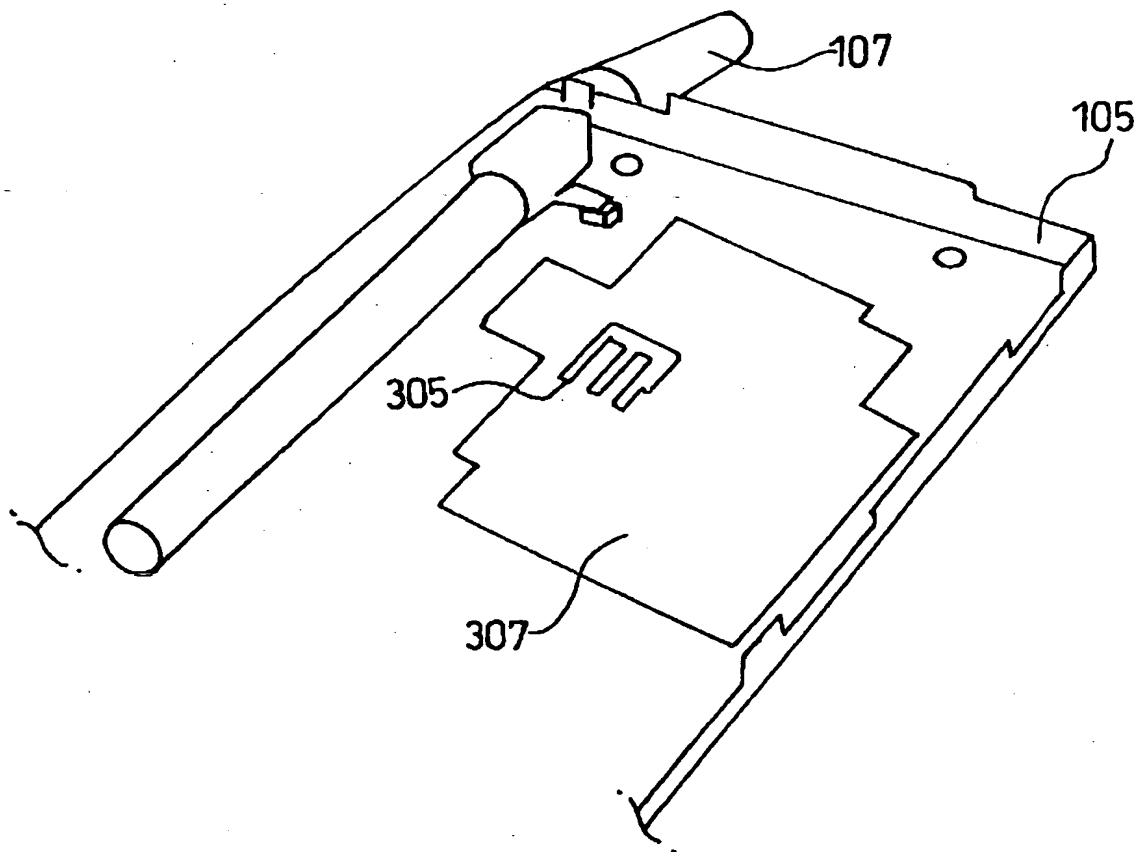

8/11

FIG. 8

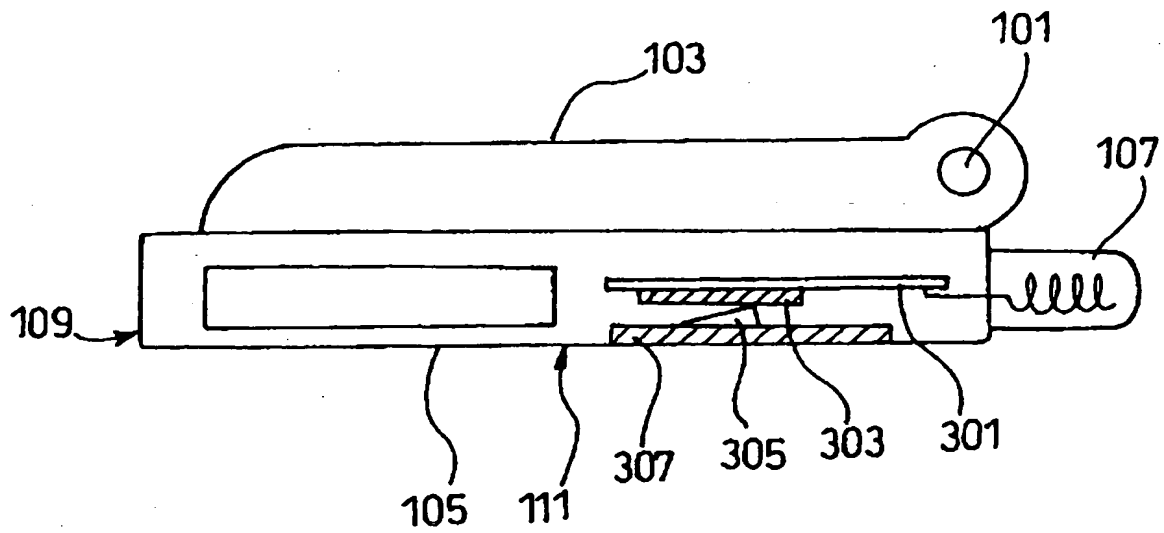



9/11

10/534153  
REPLACEMENT SHEET  
Rec'd PCT/PTO 16 JUN 2005

FIG. 9

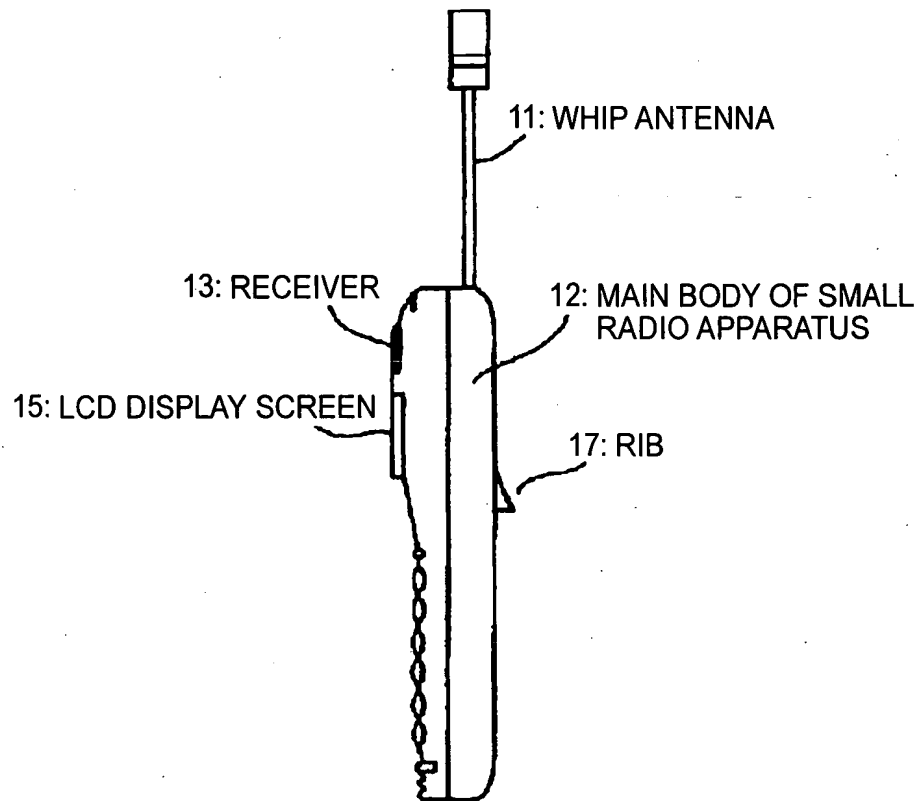


FIG. 10 (c)

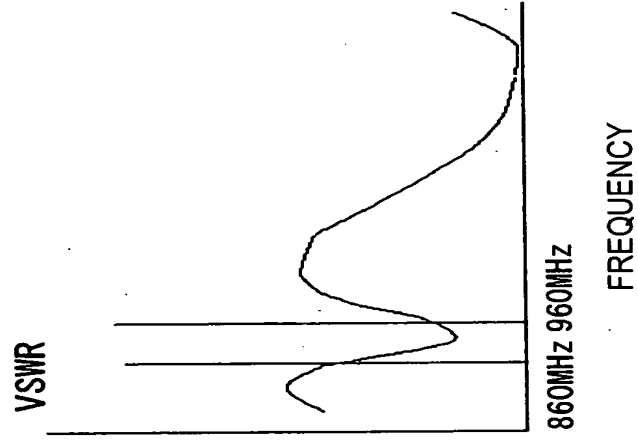


FIG. 10 (b)


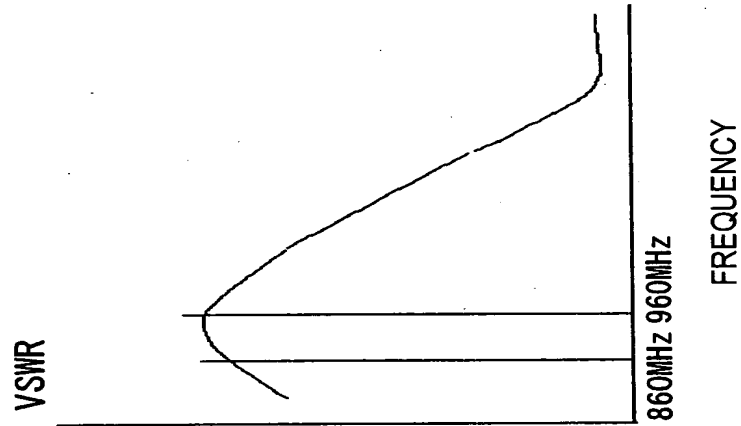


FIG. 10 (a)

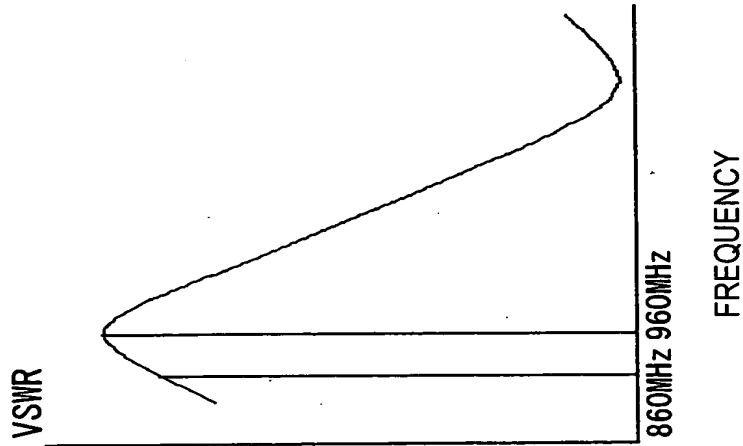

11/11

FIG. 11 (a)

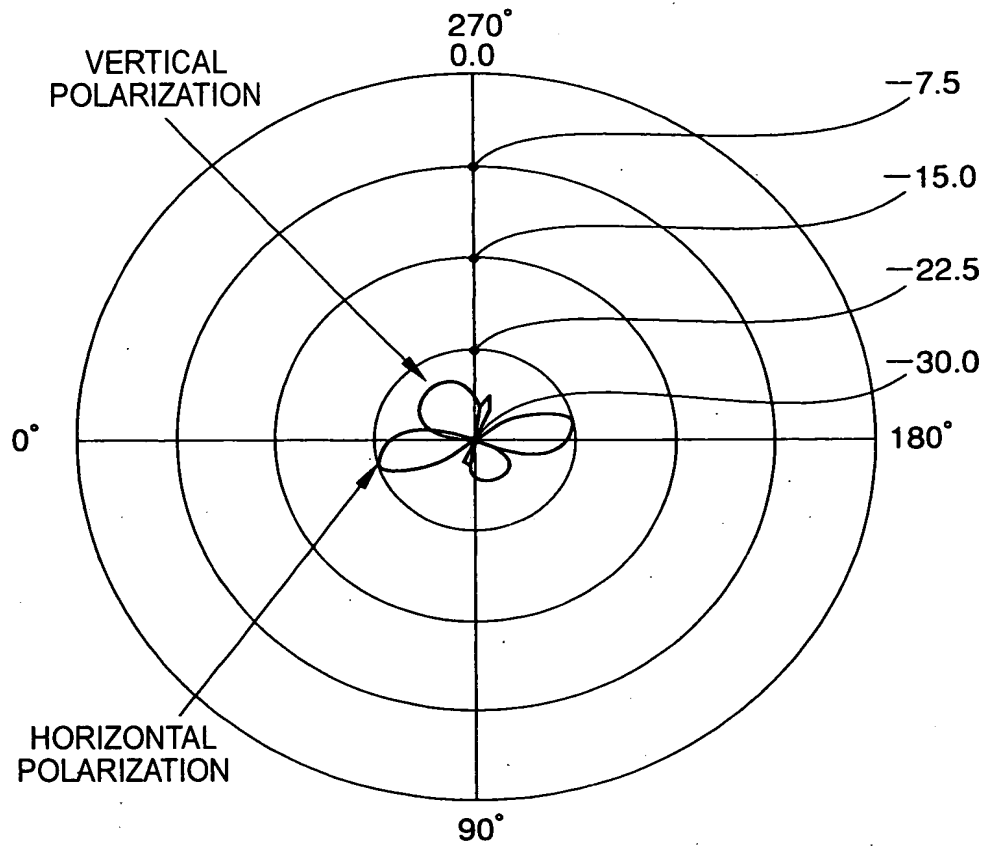


FIG. 11 (b)

